



# **A Hybrid Analysis of Machine Learning and Deep Learning Algorithms for Sleep Apnea Detection from Single-Lead ECG**

**1. Prashant K Mulge, 2. Sharanabasappa V H**

*M.Tech, Scholar, Dept. of AI & DS, Faculty of Engineering & Technology (Co-Edu.), Sharnbasva University, Kalburagi, Karnataka-India, [pachimulge@gmail.com](mailto:pachimulge@gmail.com)*

*Assistant Professor, Department of Computer Science & Engineering, Faculty of Engineering & Technology (Co-Edu.), Sharnbasva University, Kalburagi, Karnataka-India, [imsharanvh@gmail.com](mailto:imsharanvh@gmail.com)*

**ABSTRACT:** Sleep apnea (SA) is a type of sleep disorder characterized by snoring and chronic sleeplessness, which can lead to serious conditions such as high blood pressure, heart failure, and cardiomyopathy (enlargement of the muscle tissue of the heart). The electrocardiogram (ECG) plays a critical role in identifying SA since it might reveal abnormal cardiac activity. Recent research on ECG-based SA detection has focused on feature engineering techniques that extract specific characteristics from multiple-lead ECG signals and use them as classification model inputs. Machine learning and deep learning methods were applied for sleep apnea detection. Among conventional machine learning algorithms, linear and quadratic discriminate analyses, logistic regression, Gaussian naïve Bayes, Gaussian process, support-vector machine, K-nearest neighbour, decision tree, extra tree, random forest, AdaBoost, gradient boosting, multi-layer perceptron, and majority voting were implemented. Among deep algorithms, Inception v3, convolutional networks (Alex-Net, VGG16, VGG19, ZF-Net), recurrent networks (LSTM, bidirectional LSTM, gated recurrent unit), and

hybrid convolutional-recurrent networks were implemented.

The available data were divided into a training set to adjust the model parameters, a validation set to adjust hyperparameters, avoid overfitting, and improve the generalizability of the models, and a test set to evaluate the generalizability of the models on unseen data. This procedure was then repeated in a 5-fold cross-validation scheme so that all the recordings were once located in the test set. It was found that in machine learning Voting Regressor (VR) gives a highest accuracy of 78.95% among all the algorithms used. Similarly, in InceptionV3 gives a highest accuracy of 98.31% among all the DL algorithms used. This study provides valuable information on how different machine learning and deep learning algorithms perform in the detection of sleep apnea and can further be extended toward the detection of other sleep events.

***Keywords: Machine Learning, Deep Learning, Sleep Apnea, Single Lead ECG, Sleep apnea***

## INTRODUCTION

Sleep has a tremendous impact on health and quality of life, accounting for around one-third of the human life span. The two basic sleep phases are rapid eye movement (REM) and non-rapid eye movement (NREM) (NREM). REM sleep is associated with increased sympathetic activity, cardiac instability, and hemodynamic abnormalities as compared to NREM sleep. NREM is distinguished by a reduction in oxygen consumption, heart rate, and blood pressure, while REM is distinguished by an increase in all three measures. Sleep apnea may occur during any stage of sleep, although it is more common during the REM period. This is mostly because the muscles of the upper airway relax much more during the REM period of sleep. The number of people suffering from sleep problems is increasing. Sleep problems are expected to affect around 70 million people in the United States. Morbidity and death rates increase in those who have sleep disorders. Insomnia, sleep breathing disorders, central disorders of hypersomnolence, circadian rhythm sleep-wake disorders, parasomnias, and movement disorders are the most common types of sleep disorders. The most common sleep disorders are sleep breathing disorders (SBD). SBDs are classified into four types: obstructive sleep apnea (OSA), central sleep apnea (CSA), hypoventilation during sleep, and hypoxia disorders. OSA is caused by upper airway blockage, while CSA

occurs when the brain is unable to connect effectively with the breathing muscles. OSA affects one billion people globally, according to estimates. CSA occurs less commonly than other types of apnea. While OSA occurs throughout both the REM and NREM periods, it is more severe during the REM cycle, while CSA occurs mostly during the NREM cycle.

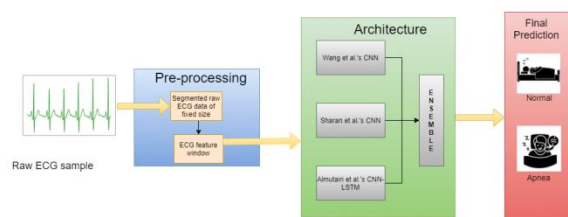


Fig.1: Example figure

Accurate, inexpensive, and portable devices that identify and monitor sleep episodes are necessary to prevent and treat cardiovascular, behavioural, and other health concerns associated with sleep apnea. There has been a significant amount of study on the creation of automated algorithms for the diagnosis of sleep apnea using a range of physiological signals, with ECG showing the most promising results in terms of both convenience and accuracy [2, 4], [5]. Apnea detection with a single-lead electrocardiogram (ECG) opens up the possibility of designing and developing wearable devices based on a single sensor.

## 1. LITERATURE REVIEW

### Detection of sleep apnea from single-lead ECG: Comparison of deep learning

### **algorithms:**

Apnea is a common sleep condition that has a negative influence on human health and quality of life. Accurate automated sleep apnea detection methods are required for assessing long-term sleep data and monitoring and managing its side effects and repercussions. Deep learning algorithms are of special relevance among diverse techniques for autonomous identification of sleep apnea using biosignals because, unlike standard machine learning algorithms, they do not depend on expert-crafted characteristics. We created and tested a variety of deep learning models for detecting sleep apnea from a single-lead electrocardiogram (ECG) data in this study. The R-peak amplitude and R-R intervals from the ECG were extracted, and power spectral analysis was used to align the R-peak amplitude and R-R intervals in frequency domain. Convolutional neural network (CNN), long short-term memory (LSTM), bidirectional LSTM, gated recurrent unit, and deep hybrid models were built and tested. Deep learning techniques were tested on an apnea-ECG dataset of 70 recordings, which was separated into a learning set of 35 records and a test set of 35 records. With a hybrid CNN and LSTM network, the best accuracy, sensitivity, specificity, and F1-score on the test data were 80.67%, 75.04%, 84.13%, and 74.72%, respectively. Deep learning studies offer potential for better apnea detection.

### **Classifier precision analysis for sleep apnea**

### **detection using ecg signals:**

This article details a research on the effectiveness of developing classifiers for the identification of sleep apnea moments based on a minute-to-minute Electrocardiogram (ECG) signal, comparing the accuracy of several classifiers. A Sgolay filter was used to each ECG signal to extract the Heart Rate Variability (HRV) and ECG-Derived Respiration (EDR), which were then utilised for classifier training, testing, and validation. In a second step, the same traits were expanded to determine if all of the categorised features were relevant. The greatest accuracy was 82.12%, with sensitivity and specificity of 88.41% and 72.29%, respectively, according to the data. This research demonstrates the significance of selecting the best classifier for a certain issue, as well as selecting and using the best features for improved accuracy. These intriguing early-stage findings may lead to more research to enhance the classifiers for potential real-world applications. The suggested model's performance was compared to previous techniques for detecting sleep apnea.

### **A novel approach osa detection using single-lead ECG scalogram based on deep neural network:**

Obstructive sleep apnea (OSA) is the most prevalent and severe breathing disorder that commonly causes breathing to stop for more than 10 seconds while sleeping. The traditional

method for treating OSA detection is polysomnography (PSG). However, this method is expensive and time-consuming. To address the aforementioned issue, an acceptable and new approach for interpreting sleep apnea utilising ECG were recording is being developed. For many years, the approaches for OSA analysis based on ECG have been studied. Early study focused on extracting traits, which are fully dependent on the expertise of human professionals. This research looks at a unique strategy for predicting sleep apnea condition based on a convolutional neural network (CNN) and a pre-trained (AlexNet) model. The 2D scalogram pictures are obtained after filtering a per-minute segment of a single-lead ECG recording using continuous wavelet transform (CWT). Finally, a CNN-based deep learning method is used to improve classification performance. The suggested model's efficiency is compared to earlier approaches that employed the same datasets. The proposed CNN-based technique achieves 86.22% accuracy and 90% sensitivity in per-minute segment OSA classification. Our study successfully classifies all aberrant apneic recordings with 100% accuracy based on per-recording OSA diagnosis. Our OSA analysis model using a time-frequency scalogram achieves good independent validation performance with several cutting-edge OSA categorization techniques. The experimental findings shown that the suggested strategy offers great performance outcomes while being minimal in cost and complexity.

### **Obstructive sleep apnea detection using convolutional neural network based deep learning framework:**

This letter describes a high-accuracy automated obstructive sleep apnea (OSA) diagnosis approach based on a deep learning framework that employs a convolutional neural network. The proposed work creates a system that analyses single lead electrocardiography data from patients and diagnoses the patient's OSA status. The findings reveal that the suggested technique has several benefits in addressing such problems, and it greatly outperforms the current methods. The current technique removes the need for separate feature extraction and classification algorithms to identify OSA. The proposed network performs feature learning as well as supervised feature classification. The system is computationally demanding, but it can reach a very high degree of accuracy—a margin of more than 9% on average when compared to other published material to date. The approach is also resistant to noise contamination of the signals. Even with pessimistic signal-to-noise ratio estimates in mind, the previously described approaches cannot outperform the current method. The software for the algorithm described here might be a strong candidate for inclusion in a module for a portable medical diagnostic system.

### 3. METHODOLOGY

The first automated approaches for detecting apnea events were standard machine learning algorithms. Due to the intricacy of physiological inputs and the limited feature extraction capacity of traditional machine learning approaches, recent research has developed toward more difficult deep learning models. Because of advancements in computing power, deep learning algorithms have outperformed their classical machine learning counterparts by being able to automatically extract the bulk of representative characteristics. The performance of the algorithms is difficult to compare owing to the range of algorithms built for the detection of sleep apnea, the numerous datasets and physiological signals used to train them, the various validation procedures, and the performance metrics used to evaluate the algorithms.

#### Disadvantages:


1. It is impossible to compare the algorithms' efficacy.
2. Because of the complexity of physiological data and the limitations of traditional machine learning algorithms in extracting features, current research has shifted toward more difficult deep learning models.

In this article, we give a fair and impartial assessment of several conventional machine learning and deep learning algorithms for

detecting the occurrence of sleep apnea using a single-lead ECG. All tests are run using the same dataset and circumstances to correctly analyse and compare the performance of different algorithms. In contrast to most research, we employed three sets of data to adjust the model hyperparameters: a training set to train the model parameters, a validation set to determine the model's optimal hyperparameters, and a test set to verify the generalizability of the produced models on unseen data.

#### Advantages:

1. It was revealed that hybrid deep models with the highest accuracy, sensitivity, and specificity perform the best in terms of detection.
2. Deep learning models outperform traditional machine learning approaches.

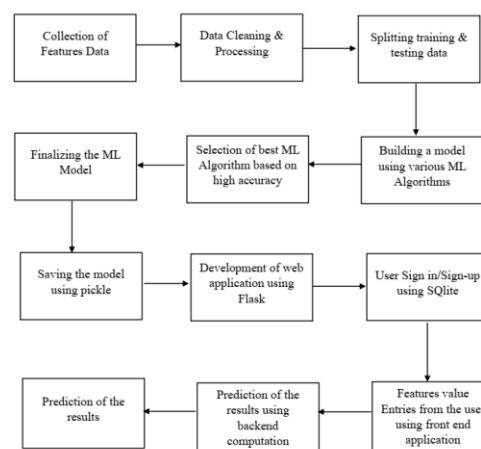

**Fig:2 System architecture for Feature data**

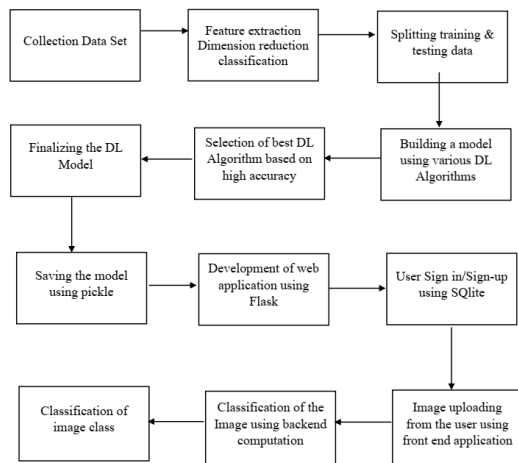


Fig:3 System architecture for Image data

Sl No	Machine Learning Model (Algorithm)	Accuracy of the model %	5-Fold cross validation mean accuracy %
1.	Linear Regression (LR)	52.16	38.61
2.	Random Forest (RF)	60.26	35.78
3.	ElasticNet (EN)	51.06	38.67
4.	Decision Tree (DT)	26.43	-38.50
5.	Majority Rule/Voting Regressor (VR)	<b>78.95</b>	<b>41.33</b>
6.	Naive Bayes (NB)	51.91	38.97
7.	Gaussian Process (GP)	51.50	39.27
8.	Support Vector Machine (SVM)	48.16	32.18
9.	KNeighbors (KN)	44.76	14.11
10.	AdaBoost (AB)	24.96	0.73
11.	Multilayer Perceptron (MLP)	54.90	40.34
12.	Gradient Boosting (GB)	59.61	40.17
13.	Stacking Regressor (SR)	11.38	9.78

Table:1 Accuracy and 5-Fold Cross validation accuracy comparison of various ML models

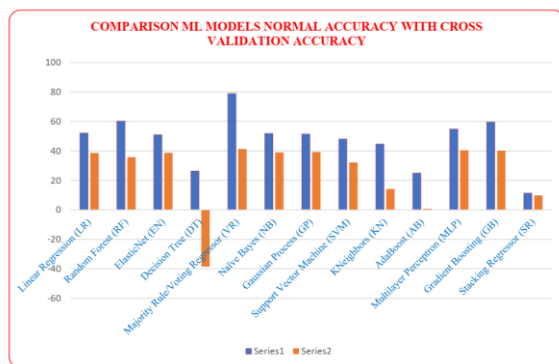


Fig:4 Comparison ML Models Normal Accuracy with Cross Validation Accuracy

Sl No	Deep Learning Model (Algorithm)	Training		Validation	
		Loss	Accuracy	Loss	Accuracy
1.	InceptionV3	<b>7.09</b>	<b>98.31</b>	<b>6.01</b>	<b>98.62</b>
2.	VGG16	95.73	76.56	95.30	74.53
3.	VGG19	88.97	77.03	92.11	75.00
4.	MobileNet	29.61	94.22	31.48	78.28
5.	ZFNet	0	0.31	0	0.31
6.	AlexNet	86.62	96.25	135.4	82.34
7.	LSTM with CNN using Xception	0	1	0	0.65
8.	BiLSTM	0	0.50	0	10.06
9.	GRU	0	0.56	0	10.06
10.	Hybrid ZFNet + LSTM	0	0.44	0	10.06
11.	Hybrid ZFNet + BiLSTM	0	0.31	0	10.06
12.	VGG16 + LSTM	0	0.81	0	10.06
13.	VGG16 + BiLSTM	0	0.88	0	10.06
14.	VGG16 + GRU	0	0.81	0	10.06
15.	VGG19 + BiLSTM	0	0.94	0	10.06

Table:7.3 Deep learning models training and validation details

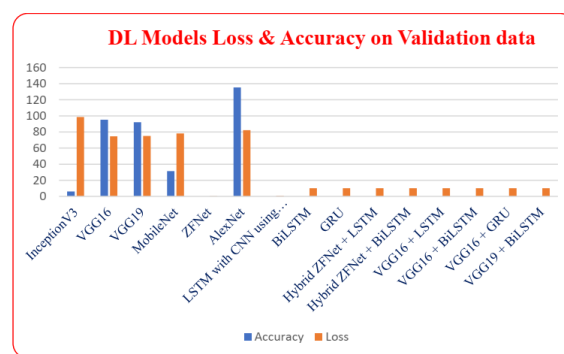


Fig:5 DL Models Loss & Accuracy on Validation data

## MODULES:

To implement aforementioned project we have created the modules listed below

1. Linear regression, Random forest, Elastic net, decision tree, nave bayes, SVM, KNN, Adaboost,MLP, Gradient boosting, Guassian process, Stacking regressor, Majority rule/Voting classifier, Linear discriminant analysis, Quadratic discriminant analysis for feature data.



2. Inceptionv3, VGG16, VGG19, MobileNet, ZFNet, AlexNet, LSTM, BiLSTM, GRU, Hybrid ZFNet (LSTM, BiLSTM, GRU), Hybrid AlexNet (LSTM, BiLSTM, GRU), Hybrid VGG16 (LSTM, BiLSTM, GRU), Hybrid VGG19 (LSTM, BiLSTM, GRU), Hybrid VGG19 (LSTM, BiLS (LSTM, BiLSTM, GRU) for image based data.

This model Inceptionv3 and voting classifier Regressor are used to forecast user input since they provide improved accuracy.

#### **4. IMPLEMENTATION**

##### **ALGORITHMS:**

**Inception V3:** Inception v3 is an image recognition model that has been shown to achieve higher than 78.1% accuracy on the ImageNet dataset. The model represents the result of several concepts explored over time by many academics. Inception v3 is a convolutional neural network that was developed as a Googlenet module to aid with picture processing and object recognition. It is the third version of Google's Inception Convolutional Neural Network, which was first unveiled as part of the ImageNet Recognition Challenge.

**VGG16:** VGG-16 is a 16-layer convolutional neural network. A pretrained version of the network trained on over a million photos from the ImageNet database may be loaded [1]. The pretrained network can categorise photos into 1000 different item categories, including

keyboards, mice, pencils, and other animals. It is regarded as one of the best vision model architectures to date. The most distinguishing feature of VGG16 is that instead of a huge number of hyper-parameters, they concentrated on having convolution layers of 3x3 filter with stride 1 and always utilised the same padding and maxpool layer of 2x2 filter with stride 2.

**VGG19:** VGG19 is a VGG model version that consists of 19 layers (16 convolution layers, 3 Fully connected layer, 5 MaxPool layers and 1 SoftMax layer). Other VGG variations include VGG11, VGG16, and more. VGG19 has a total of 19.6 billion FLOPs. VGG19 is a sophisticated CNN with pre-trained layers and a strong grasp of what constitutes an image in terms of form, colour, and structure. VGG19 is a highly deep neural network that has been trained on millions of photos with challenging classification tasks.

**MobileNet:** A convolutional neural network (CNN) built for mobile and embedded vision applications. They are based on a simplified design that use depthwise separable convolutions to construct lightweight deep neural networks with reduced latency for mobile and embedded devices. MobileNets are a subset of convolutional neural networks that are tiny, low-latency, and low-power models that may be used for categorization, detection, and other common tasks. Because of their compact size, these deep learning models are ideal for application on mobile devices.

**ZFNet:** ZFNet is a traditional convolutional neural network. Visualizing intermediate feature layers and the functioning of the classifier inspired the design. When compared to AlexNet, the filter widths and stride of the convolutions are lowered. It had five shared convolutional layers, four max-pooling layers, three dropout layers, and three fully connected layers. In the first layer, it employed a 77 size filter and a lower stride value. The softmax layer is ZFNet's last layer.

**AlexNet:** AlexNet is an 8-layer convolutional neural network. A pretrained version of the network trained on over a million photos from the ImageNet database may be loaded. The pretrained network can categorise photos into 1000 different item categories, including keyboards, mice, pencils, and other animals. The Alexnet includes eight levels of parameters that may be learned. The model is composed of five layers, the first of which is a max pooling layer, followed by three fully connected layers, and each of these levels, save the output layer, uses Relu activation.

**LSTM:** LSTM is an abbreviation for long short-term memory networks, which are utilised in Deep Learning. It is a kind of recurrent neural networks (RNNs) that may learn long-term dependencies, particularly in sequence prediction tasks. LSTMs use a number of 'gates' that regulate how information in a data sequence enters, is stored in, and exits the network. A typical LSTM has three gates: a forget gate, an

input gate, and an output gate. These gates function as filters and each have their own neural network.

**BiLSTM:** A bidirectional LSTM (BiLSTM) layer learns the bidirectional long-term relationships between time steps in a time series or sequence data. When you want the network to learn from the whole time series at each time step, these dependencies might be advantageous. More particular, it was discovered that BiLSTM models outperform ARIMA and LSTM models in terms of prediction. BiLSTM models were likewise shown to attain equilibrium substantially slower than LSTM-based models. Forecasting is an important yet difficult aspect of time series data research.

**GRU:** Gated recurrent units (GRUs) are a recurrent neural network gating technique established in 2014 by Kyunghyun Cho et al. The GRU functions similarly to a long short-term memory (LSTM) with a forget gate, but with fewer parameters since it lacks an output gate. The Gated Recurrent Unit (GRU) is a form of Recurrent Neural Network (RNN) that offers benefits over long short term memory (LSTM) in certain instances. GRU consumes less memory and is quicker than LSTM, although LSTM is more accurate when utilising datasets with longer sequences.



## 5. EXPERIMENTAL RESULTS

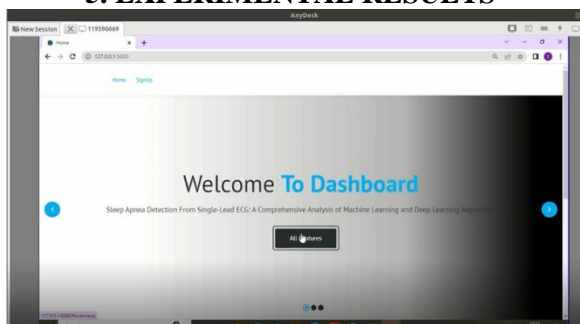


Fig.3: Home screen

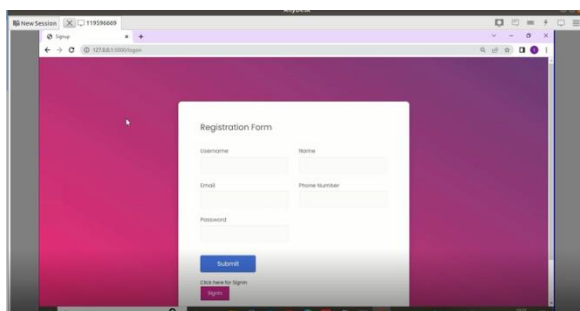


Fig.4: User registration

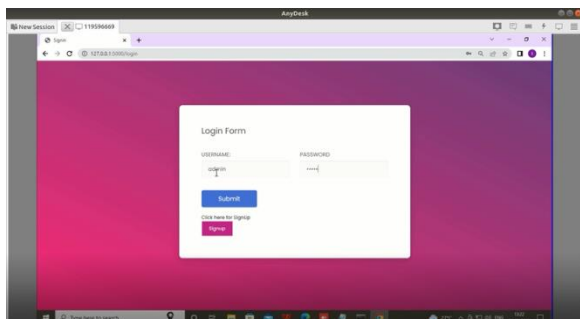


Fig.5: user login

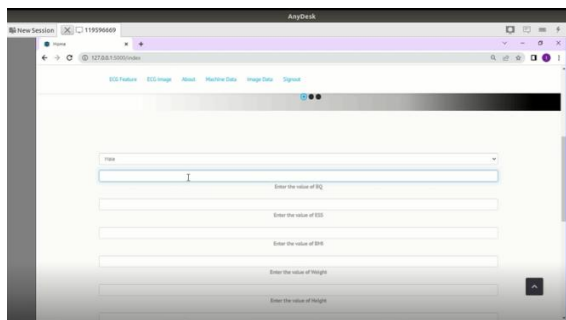


Fig.6: Main screen

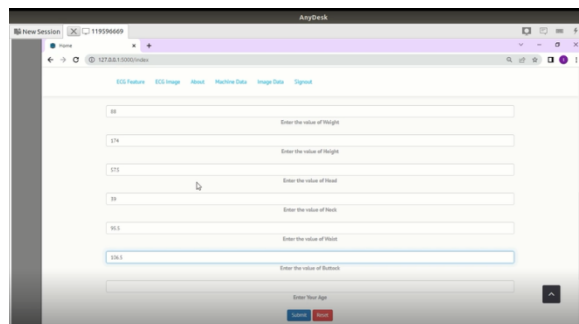


Fig.7: User input

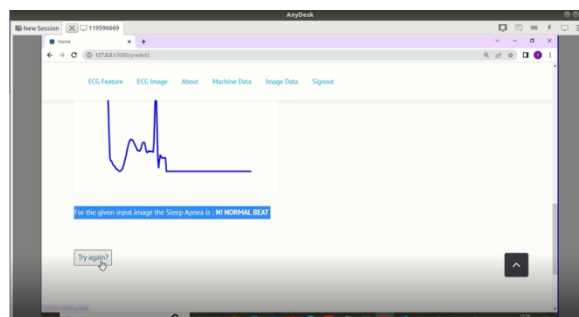


Fig.8: Prediction result

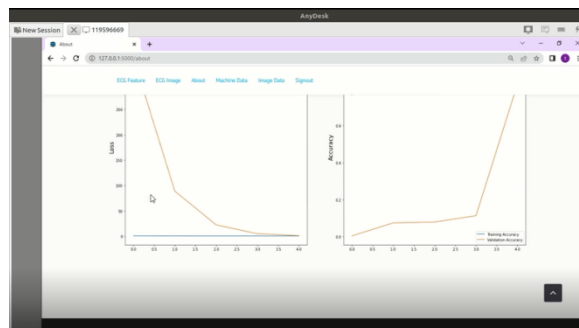


Fig.9: Accuracy graph

## 6. CONCLUSION

In this paper a comprehensive comparison between different machine learning and deep learning algorithms for the detection of sleep apnea from single-lead ECG analysed. Several machine learning

and deep learning classifiers were employed to diagnose the OSA. The performances of the proposed models were validated and tested using the ECG dataset and ECG images. Among the machine learning classifiers, our results indicated that the Voting regressor contributed to the highest performance. Similarly in deep learning inception V3 contributed to the highest performance. This work provides valuable information to sleep apnea researchers on the design and selection of appropriate machine learning and deep learning algorithms for the detection of sleep apnea.

#### **REFERENCES**

- [1] M. Bahrami and M. Forouzanfar, "Detection of sleep apnea from single-lead ECG: Comparison of deep learning algorithms," in 2021 IEEE International Symposium on Medical Measurements and Applications (MeMeA), 2021: IEEE, pp. 1-5.
- [2] N. Pombo, B. M. Silva, A. M. Pinho, and N. Garcia, "Classifier precision analysis for sleep apnea detection using ecg signals," *IEEE Access*, vol. 8, pp. 200477-200485, 2020.
- [3] M. H. Kryger, T. Roth, and W. C. Dement, *Principles and Practice of sleep medicine*, 6th Edition ed. Elsevier Inc., 2017.
- [4] S. A. Singh and S. Majumder, "A novel approach osa detection using single-lead ECG scalogram based on deep neural network," *Journal of Mechanics in Medicine and Biology*, vol. 19, no. 04, p. 1950026, 2019.
- [5] D. Dey, S. Chaudhuri, and S. Munshi, "Obstructive sleep apnoea detection using convolutional neural network based deep learning framework," *Biomedical engineering letters*, vol. 8, no. 1, pp. 95- 100, 2018.
- [6] J. Acquavella, R. Mehra, M. Bron, J. M.-H. Suomi, and G. P. Hess, "Prevalence of narcolepsy and other sleep disorders and frequency of diagnostic tests from 2013–2016 in insured patients actively seeking care," *J. Clin. Sleep Med.*, vol. 16, no. 8, pp. 1255-1263, 2020.
- [7] O. Faust, R. Barika, A. Shenfield, E. J. Ciaccio, and U. R. Acharya, "Accurate detection of sleep apnea with long short-term memory network based on RR interval signals," *Knowledge-Based Systems*, vol. 212, p. 106591, 2021.
- [8] B. M. Altevogt and H. R. Colten, "Sleep disorders and sleep deprivation: an unmet public health problem," Washington (DC): National Academies Press (US), 2006.
- [9] K. Feng, H. Qin, S. Wu, W. Pan, and G. Liu, "A Sleep Apnea Detection Method Based on Unsupervised Feature Learning and Single-Lead Electrocardiogram," *IEEE Transactions on Instrumentation and Measurement*, vol. 70, pp. 1-12, 2020.

[10] A. B. Neikrug and S. Ancoli-Israel, "Sleep disorders in the older adult—a mini-review," *Gerontology*, vol. 56, no. 2, pp. 181-189, 2010.

[11] Q. Shen, H. Qin, K. Wei, and G. Liu, "Multiscale Deep Neural Network for Obstructive Sleep Apnea Detection Using RR Interval From Single-Lead ECG Signal," *IEEE Transactions on Instrumentation and Measurement*, vol. 70, pp. 1-13, 2021.

[12] M. M. Lyons, N. Y. Bhatt, A. I. Pack, and U. J. Magalang, "Global burden of sleep-disordered breathing and its implications," *Respirology*, vol. 25, no. 7, pp. 690-702, 2020.

[13] A. Pinho, N. Pombo, B. M. Silva, K. Bousson, and N. Garcia, "Towards an accurate sleep apnea detection based on ECG signal: The quintessential of a wise feature selection," *Applied Soft Computing*, vol. 83, p. 105568, 2019.

[14] W. Conwell et al., "Prevalence, clinical features, and CPAP adherence in REM-related sleep-disordered breathing: a cross sectional analysis of a large clinical population," *Sleep and Breathing*, vol. 16, no. 2, pp. 519-526, 2012.

[15] B. Fatimah, P. Singh, A. Singhal, and R. B. Pachori, "Detection of apnea events from ECG segments using Fourier decomposition method," *Biomed. Signal Process. Control*, vol. 61, p. 102005, 2020.